



Contour[®] plus ONE⁾⁾

Blood Glucose
Monitoring System

Testing your blood glucose for the first time with the **CONTOUR®PLUS ONE** smart meter




Always consult with your healthcare provider prior to making changes to treatment, diet or exercise.


© Copyright 2017 Ascensia Diabetes Care Holdings AG

Contour.
plus **ONE**»
Blood Glucose
Monitoring System


diabetes.ascensia.com




The **CONTOUR PLUS ONE** meter has been shown to provide highly accurate blood glucose results.

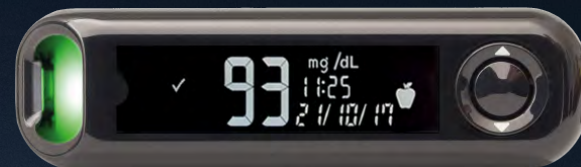

Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System



Initial
CONTOUR PLUS ONE
meter setup

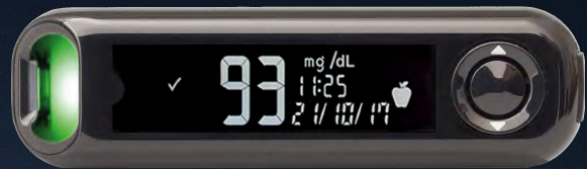

Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System




Initial Setup


Before you test, this meter requires a simple initial Setup.

Unlock the benefits in 3 simple steps.

Press and hold the 'OK' button for 2 seconds until the meter turns on.

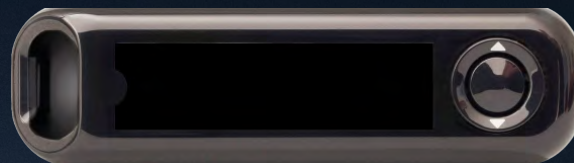

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System




Initial Setup


Before you test, this meter requires a simple initial Setup.

Unlock the benefits in 3 simple steps.

Press and hold the 'OK' button for 2 seconds until the meter turns on.

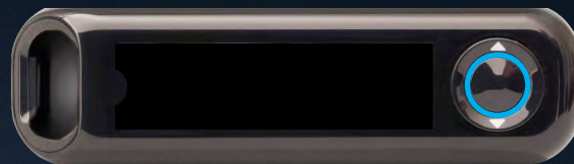

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System




Initial Setup


Before you test, this meter requires a simple initial Setup.

Unlock the benefits in 3 simple steps.

Press and hold the 'OK' button for 2 seconds until the meter turns on.

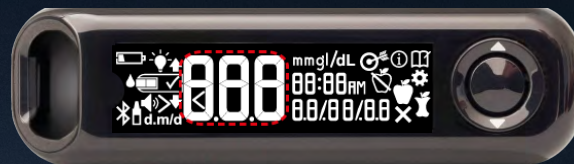

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



1.

Initial Setup


Note and accept the Target Ranges*.
Press the 'OK' button.

* You can change the pre-set Target Range from the **CONTOUR DIABETES app** after initial setup of the meter.

WARNING - Talk to your Health Care Professional before setting or changing any Target Ranges in the **CONTOUR DIABETES app**.



Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System



1.

Initial Setup


Note and accept the Target Ranges*.
Press the 'OK' button.

* You can change the pre-set Target Range from the **CONTOUR DIABETES app** after initial setup of the meter.

WARNING - Talk to your Health Care Professional before setting or changing any Target Ranges in the **CONTOUR DIABETES app**.



Contour
plus **ONE**
Blood Glucose
Monitoring System



2.

Initial Setup

Confirm or adjust the time on the meter.


To change the hour, press the ▲ or ▼ button on the outer ring.

To set the hour and move to minutes, press the 'OK' button.

To change the minutes, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



2.

Initial Setup

Confirm or adjust the time on the meter.


To change the hour, press the ▲ or ▼ button on the outer ring.

To set the hour and move to minutes, press the 'OK' button.

To change the minutes, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



2.

Initial Setup

Confirm or adjust the time on the meter.

To change the hour, press the ▲ or ▼ button on the outer ring.

To set the hour and move to minutes, press the 'OK' button.

To change the minutes, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



2.

Initial Setup

Confirm or adjust the time on the meter.


To change the hour, press the ▲ or ▼ button on the outer ring.

To set the hour and move to minutes, press the 'OK' button.

To change the minutes, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.


Initial Setup

Confirm or adjust the date on the meter


To change the year, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the month, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the day, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

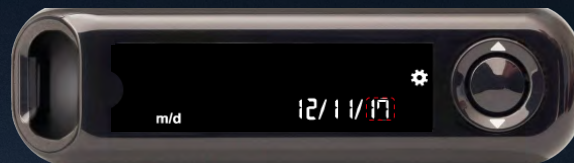

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.

Initial Setup

Confirm or adjust the date on the meter


To change the year, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the month, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the day, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.


Initial Setup

Confirm or adjust the date on the meter


To change the year, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the month, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the day, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

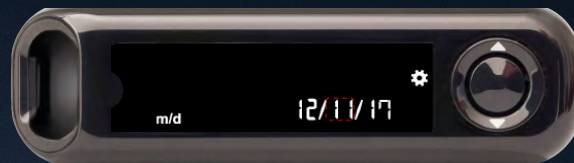

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.


Initial Setup

Confirm or adjust the date on the meter


To change the year, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the month, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the day, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

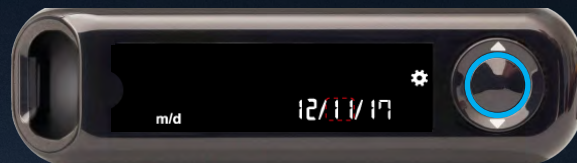

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.


Initial Setup

Confirm or adjust the date on the meter


To change the year, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the month, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the day, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

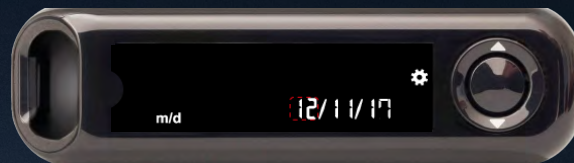

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.


Initial Setup

Confirm or adjust the date on the meter


To change the year, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the month, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

To change the day, press the ▲ or ▼ button on the outer ring. Press the 'OK' button.

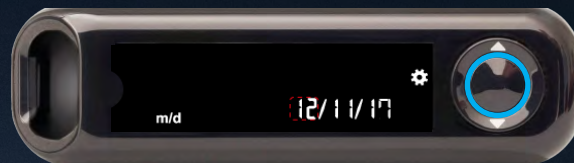

Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



4.

Initial Setup.

The meter briefly displays your saved settings, then beeps and turns off.

Setup is complete. You are ready to test your blood glucose.




Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System

Testing
your blood glucose with
the **CONTOUR PLUS ONE**
meter



Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System





1.


Insert the test strip

Hold the test strip with the grey square end facing toward the meter.

Insert the grey square end firmly into the test strip port until the meter beeps.

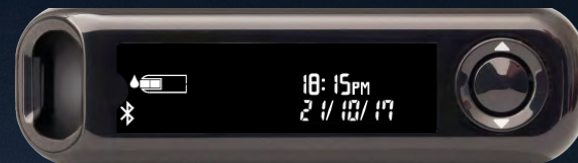

Contour[®]
plus **ONE** »
Blood Glucose
Monitoring System



1.


Insert the test strip

Hold the test strip with the grey square end facing toward the meter.

Insert the grey square end firmly into the test strip port until the meter beeps.



Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System



2.


Apply blood

The test strip icon flashes when the meter is ready to test a blood drop.


Immediately touch the tip of the test strip to the drop of blood.

The blood is drawn into the test strip through the tip.

Hold the tip of the test strip in the blood drop until the meter beeps.

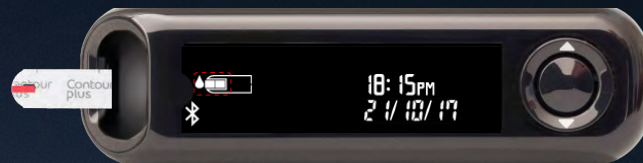

Contour[®]
plus **ONE** »
Blood Glucose
Monitoring System



3.


Results

After a 5 second count down the meter displays your blood glucose result.

If the Meal Marker feature is on, a Fasting, Before Meal, After Meal, or No Mark marker will blink on the blood glucose result screen.



Contour[®]
plus **ONE** »
Blood Glucose
Monitoring System



3.


Results

After a 5 second count down the meter displays your blood glucose result.

If the Meal Marker feature is on, a Fasting, Before Meal, After Meal, or No Mark marker will blink on the blood glucose result screen.



Contour[®]
plus **ONE** »
Blood Glucose
Monitoring System



3.


Results

After a 5 second count down the meter displays your blood glucose result.

If the Meal Marker feature is on, a Fasting, Before Meal, After Meal, or No Mark marker will blink on the blood glucose result screen.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System



3.

Results

After a 5 second count down the meter displays your blood glucose result.

If the Meal Marker feature is on, a Fasting, Before Meal, After Meal, or No Mark marker will blink on the blood glucose result screen.



Contour[®]
plus ONE[»]
Blood Glucose
Monitoring System




3.


Results

After a 5 second count down the meter displays your blood glucose result.

If the Meal Marker feature is on, a Fasting, Before Meal, After Meal, or No Mark marker will blink on the blood glucose result screen.

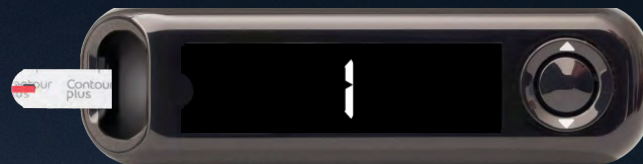

Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System




3.

Results

After a 5 second count down the meter displays your blood glucose result.

If the Meal Marker feature is on, a Fasting, Before Meal, After Meal, or No Mark marker will blink on the blood glucose result screen.

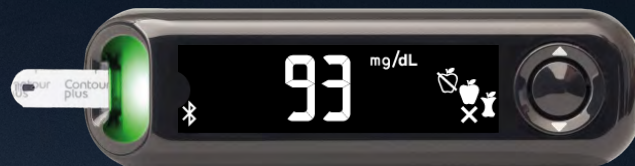

Contour[®]
plus **ONE** »
Blood Glucose
Monitoring System


4.

Results

The meter suggests a Meal Marker based on the time of day and the meal period: fasting/breakfast, lunch, dinner, or overnight.

Use the ▲ or ▼ to select the correct marker and press 'OK'.

You can select a Meal Marker for your blood glucose reading on your meter or in the **CONTOUR DIABETES app**.

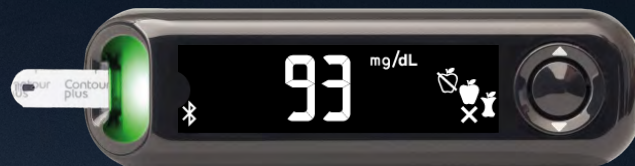

Contour[®]
plus **ONE**[»]
Blood Glucose
Monitoring System


4.

Results


The meter suggests a Meal Marker based on the time of day and the meal period: fasting/breakfast, lunch, dinner, or overnight.

Use the ▲ or ▼ to select the correct marker and press 'OK'.

You can select a Meal Marker for your blood glucose reading on your meter or in the **CONTOUR DIABETES app**.

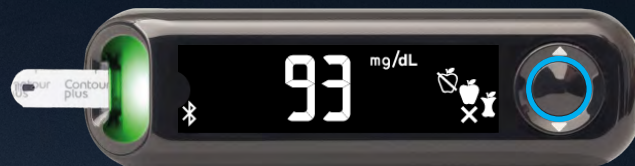

Contour[®]
plus ONE[™]
Blood Glucose
Monitoring System



5.

Results

When your blood glucose test is complete, the meter displays your results with the units, time, date, meal marker (if selected), and target indicator.

The smarLIGHT™ feature is **green** for In Target, **red** for Below Target and **yellow** for Above Target.




Contour[®]
plus **ONE**»
Blood Glucose
Monitoring System

6.

Results

The **CONTOUR DIABETES app** displays your latest result on your mobile device along with information to help manage your diabetes.

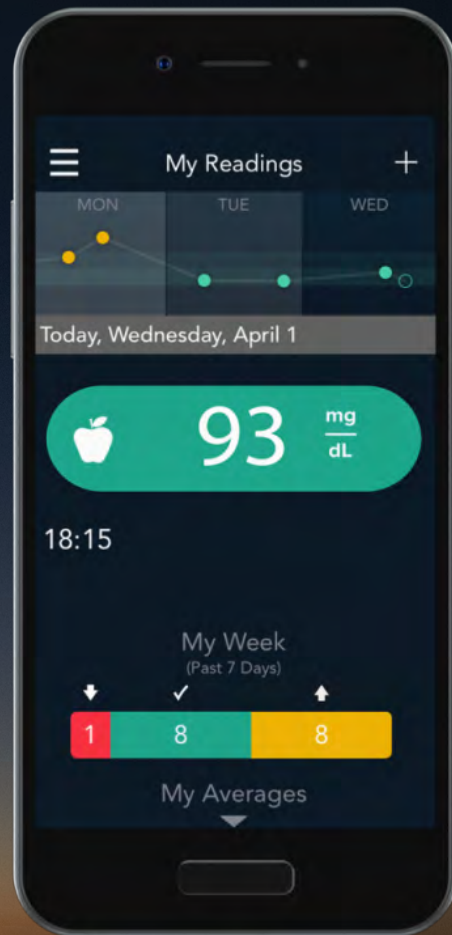


Contour
plus **ONE**
Blood Glucose
Monitoring System

diabetes.ascensia.com

Talk to your Healthcare Professional and refer to the product user guide if you have questions about the **CONTOUR®PLUS ONE** smart meter and the **CONTOUR™DIABETES app**.

For more information, and to find out whether these products are available in your country, visit diabetes.ascensia.com.

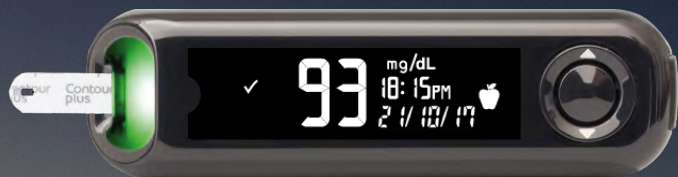

Always consult with your healthcare provider prior to making changes to treatment, diet or exercise.

Get the app




Apple and the Apple logo are trademarks of Apple Inc., registered in the US and other countries. App Store is a service mark of Apple Inc. The Bluetooth word mark and logos are registered trademarks owned by Bluetooth SIG, Inc., and any use of such marks herein is under license. Google play and the Google Play logo are trademarks of Google Inc.

Ascensia, the Ascensia Diabetes Care logo and Contour are trademarks and/or registered trademarks of Ascensia Diabetes Care Holdings AG.

Date of preparation: February 2018 code: G.DC.12.2017.52592

© Copyright 2017 Ascensia Diabetes Care Holdings AG

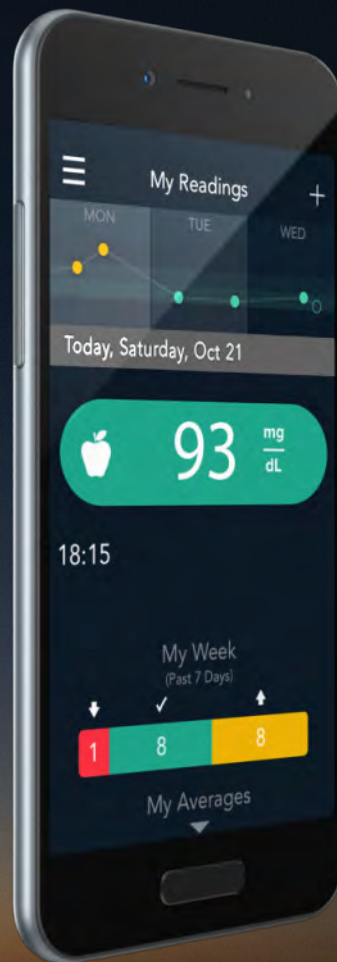

Contour
plus ONE
Blood Glucose
Monitoring System

diabetes.ascensia.com



Contour[®]

diabetes solutions